VIGA GEMILANG DIAGNOSTICS SDN BHD

B-G-8 RAWANG IDAMAN, JALAN IDAMAN 1, TAMAN RAWANG IDAMAN,
48000 RAWANG SELANGOR DARUL EHSAN

ViTEST

HCV RAPID TEST KIT (FOR PROFESSIONAL USE)

Specification
20 TESTS

Storage condition
4-30 °C

Testing time
15 minutes

Shelf life
24 months

Description

Intended use	This kit is intended for use as an aid in the diagnosis of HCV infection.
Sample	Whole Blood/Serum/Plasma
Specification	20 Tests
Storage condition	4°C-30 °C, keep dry, away from direct sunlight
Shelf life	18 months, single use




OPERATION PROCESS

1. Bring the pouch to room temperature before opening. Remove the test device from the sealed pouch and use it as soon as possible.

2. Place the test on a clean, level surface. Label with specimen ID.

For venous whole blood specimens:
Hold the dropper vertically and transfer 2 drops of whole blood (approximately 50 µL) to the sample well (S) of the test, then add 1 drop of buffer (approximately 40 µL) and start the timer.
For fingerstick whole blood specimens:
Dispense 2 drops of fingerstick whole blood onto the sample well (S) of the test, then add 1 drop of buffer (approximately 40 µL) and start the timer.
For serum or plasma specimens:
Hold the dropper vertically and transfer 3 drops of serum or plasma (approximately 75 µL) to the sample well (S) of the test and start the timer.
Avoid trapping air bubbles in the specimen well (S), and do not add any solution to the result area.

3. Wait for the colored band(s) to appear. Read results at 15 minutes.

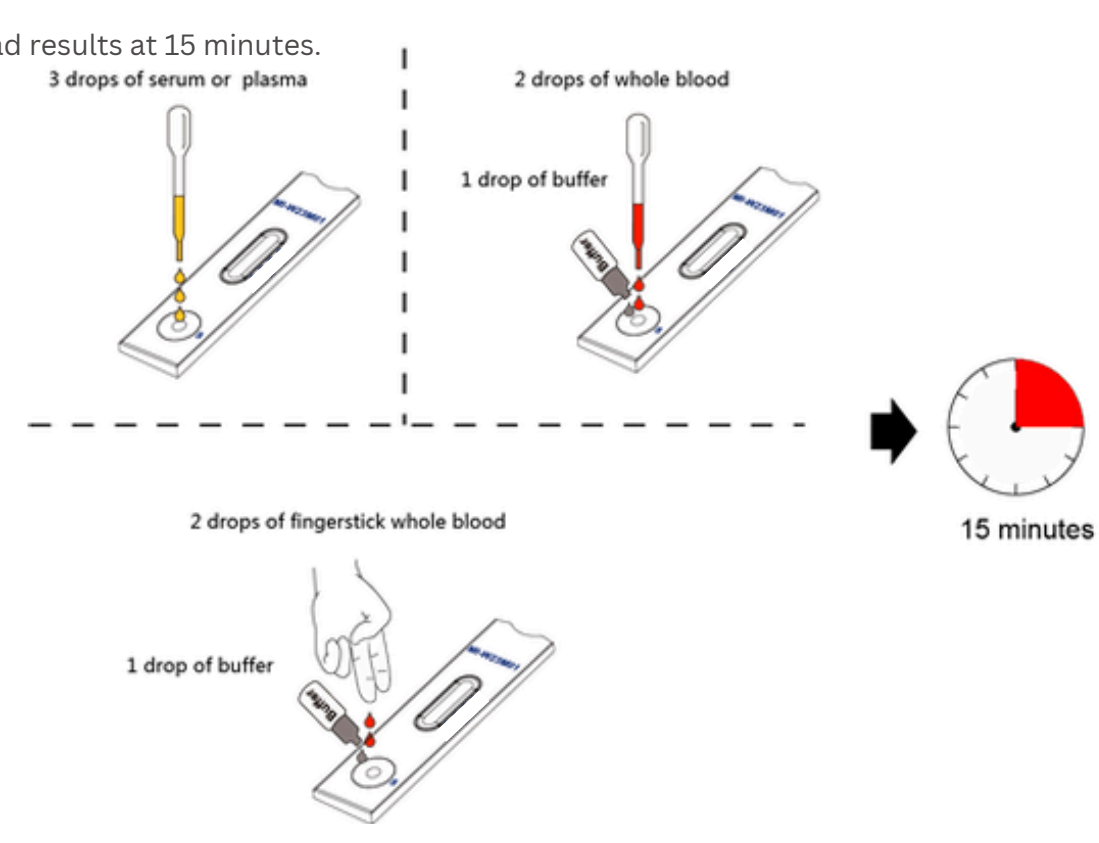

Manufacture by:
VIGA GEMILANG DIAGNOSTICS SDN BHD
B-G-8 RAWANG IDAMAN, JALAN IDAMAN 1, TAMAN RAWANG IDAMAN, 48000 RAWANG SELANGOR DARUL EHSAN
Phone Number : 012 - 313 3081 Email: sales@vigagemilang.com.my