VIGA GEMILANG DIAGNOSTICS SDN BHD
B-G-8 RAWANG IDAMAN, JALAN IDAMAN 1, TAMAN RAWANG IDAMAN,
48000 RAWANG SELANGOR DARUL EHSAN

ViTEST

FECAL OCCULT BLOOD RAPID TEST

S	**Sample**	°C	**Storage condition**	5	**Testing time**	24	**Shelf life**
	Stool / Feces		2-30 °C		5 minutes		24 months


Description




Intended use	The Fecal Occult Blood Rapid Test is designed for the qualitative detection of human occult blood in feces using a rapid immunochromatographic method. It may be used as a screening aid for gastrointestinal bleeding.
Sample	Fresh stool / feces specimen
Storage condition	2-30 °C, keep dry, avoid light and heat
Shelf life	24 months
Result reading	Read within 5 minutes

Test Procedure

1. **Collect sample:** Collect feces from different parts using the collection stick and mix sufficiently.
2. **Prepare sample:** Use fresh sample when possible. Test within 1 hour after processing.
3. **Apply sample:** Add 2 drops (80-100 µL) of diluted sample to the sample area/well.
4. **Read result:** Observe the result within 5 minutes. Do not interpret after 5 minutes.

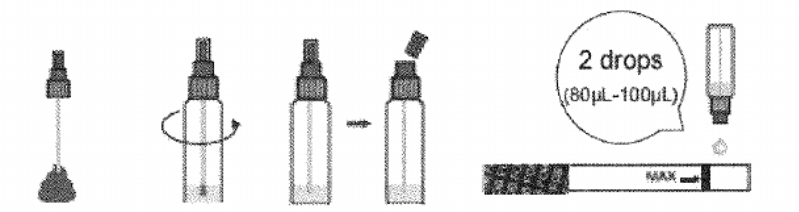

Interpretation of Results



Positive: C and T lines visible
Negative: C line only
Invalid: No C line - repeat with a new test

Manufactured by: VIGA GEMILANG DIAGNOSTICS SDN BHD
B-G-8 Rawang Idaman, Jalan Idaman 1, Taman Rawang Idaman, 48000 Rawang, Selangor Darul Ehsan
Phone: 012-313 3081 Email: sales@vigagemilang.com.my

STORE AT 2-30 °C