VIGA GEMILANG DIAGNOSTICS SDN BHD
B-G-8 RAWANG IDAMAN, JALAN IDAMAN 1, TAMAN RAWANG IDAMAN,
48000 RAWANG SELANGOR DARUL EHSAN

ViTEST

COVID & INFLUENZA A+B COMBO RAPID TEST CASSETTE

(NASOPHARYNGEAL SWAB/ NASOPHARYNGEAL WASH/ NASAL ASPIRATE)

Specification
25pcs

Storage condition
2-30 °C


Testing time
15 minutes

Shelf life
24 months

Description

Intended use	The Vitest Covid & Influenza A+B Combo Rapid Test Cassette is a rapid chromatographic immunoassay for the qualitative detection of Adenovirus antigen, Respiratory Syncytial Virus antigen and Influenza A and B antigens in nasopharyngeal swab/ Nasopharyngeal Wash/ Nasal Aspirate specimens. It is intended to aid in the rapid differential diagnosis of Adenovirus, Respiratory Syncytial Virus viral, Influenza A and B infections.
Sample	Nasopharyngeal Swab
Specification	25 pcs/box
Storage condition	2°C-30 °C, keep dry, away from direct sunlight
Shelf life	24 months, single use



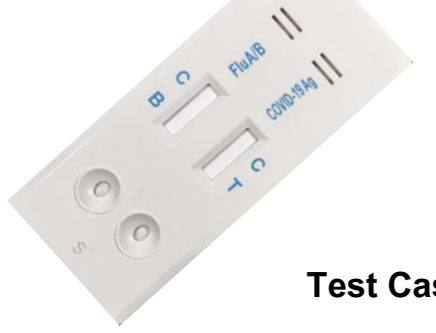

Test Cassette



Sampling Swab



Buffer




Workstation

COMPONENTS	TEST CASSETTE	SAMPLING SWAB	BUFFER	WORKSTATION	PRODUCT INSERT
25 PC/ BOX	20	20	20	1	1

OPERATION PROCESS

Bring devices, reagents and specimens and/or controls to room temperature (15~30°C) before use.

1. For each specimen, open the foil pouch just before testing and remove the test device, and put it on a clean, level surface. Label the tube with the patient identification. For best results, the assay should be performed within one hour.
2. Peel off the aluminum foil cover of the extraction buffer .
3. Insert the extraction buffer into the tube stand.
4. Insert the swab into the extraction tube. Mix well and squeeze the swab 1 0-15 times by compressing the walls of the tube against the swab. 5. Roll the swab head against the inner wall of the tube as you remove it. Try to release as much liquid as possible. Dispose of the used swab in accordance with your biohazard waste disposal protocol.
6. Insert nozzle into extraction tube. Invert the tube and add 3 drops of solution into each sample wells by gently squeezing the tube. 7. Read results at 15 minutes. Do not read the results after 20 minutes.

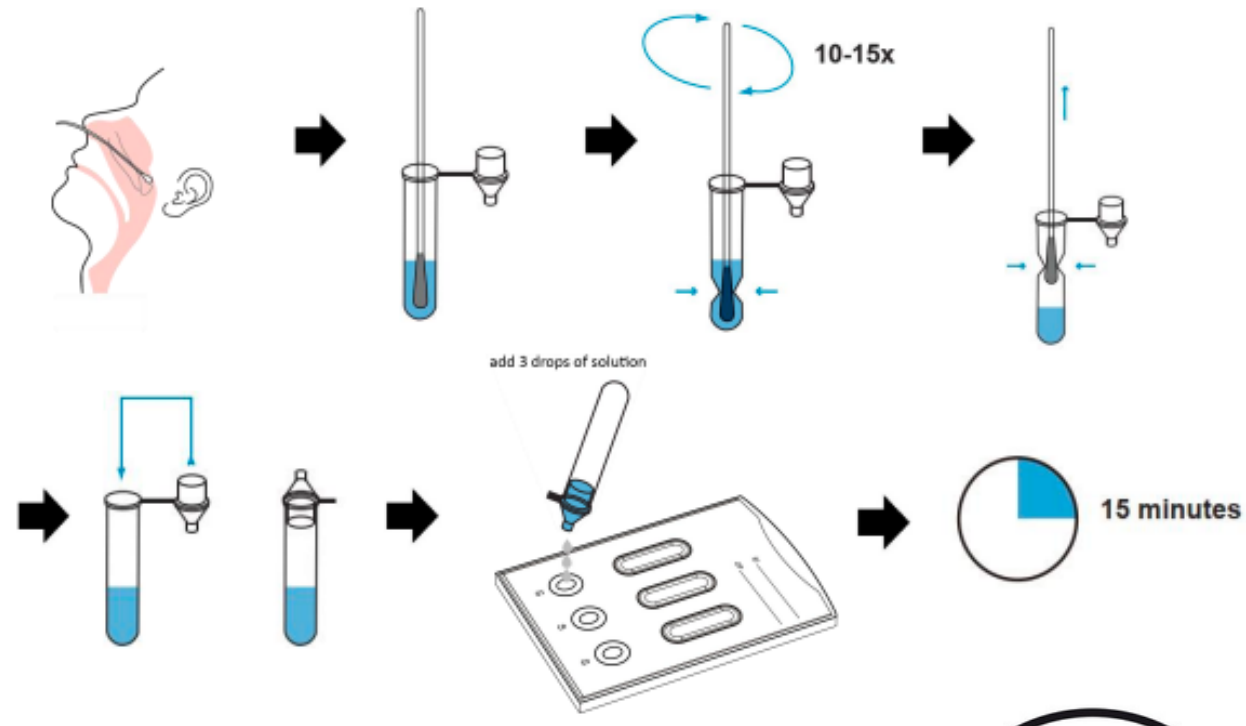

Manufacture by:
VIGA GEMILANG DIAGNOSTICS SDN BHD
B-G-8 RAWANG IDAMAN, JALAN IDAMAN 1, TAMAN RAWANG IDAMAN, 48000 RAWANG SELANGOR DARUL EHSAN
Phone Number : 012 - 313 3081 Email: sales@vigagemilang.com.my